


Hospital Grade NEMA 5-15P to IEC C13 Power Cord - 16 AWG, 13A/125V, SJT, Clear


P1:	M-005B
P2:	M-Y087A
	M-087A
P3:	M-087B

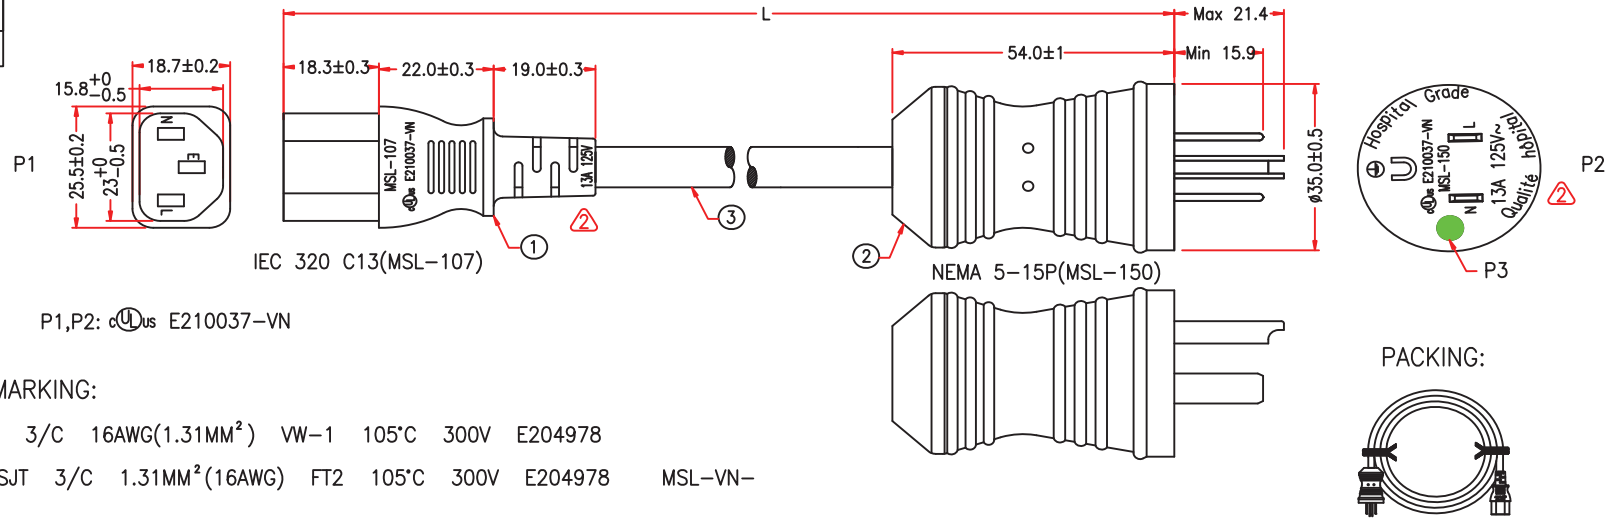

P1,P2: cULus E210037-VN

CABLE MARKING:

⚠ ⚠ (UL) SJT 3/C 16AWG(1.31MM²) VW-1 105°C 300V E204978
 C(UL) SJT 3/C 1.31MM²(16AWG) FT2 105°C 300V E204978 MSL-VN-

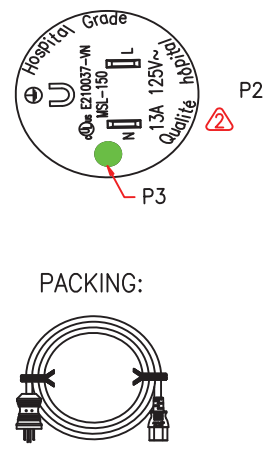

107150B2F16A(FP326-00)			
	P1		P2
BLACK	L	_____	L
WHITE	N	_____	N
GREEN	E	_____	E

Cable Length Unless Other Spec.
 Tolerances:
 0 ~200mm ±10mm
 201~1000mm ±20mm
 1001 ~1500mm ±25mm
 1501~2100mm ±30mm
 2100mm↑ ±40mm

NOTE: All relevant materials are complied with RoHS directive .
 THE CABLE MARKING IS CONCAVE LETTERING MOULD

3	UL SJT 16AWG x 3C, OD 8.5mm, JACKET GRAY(PANTONE COOL GRAY 9C)	Xmm	M304
2	MOLDED PVC 80P, COLOR GREEN		M304
	MOLDED PVC 45P, COLOR TRANSPARENT BLUE		M304
	MOLDED PVC 35P, COLOR TRANSPARENT BLUE		M304
	RIVETING CLAW	1	M1220
	TERMINAL: 98478BL-1	1	M257
1	TERMINAL: 98693BL-1	2	M257
	MOLDED PVC 35P, COLOR TRANSPARENT BLUE		M304
	BRACKET: YS-003	1	M767
	TERMINAL: 2*4mm, 98740BS-0/A	3	M257

ITEM NO.	8-PCDHG1513C-XX-16	UNIT:mm		
----------	--------------------	---------	--	--

- ⚠ REV.3 2025.01.03 | MODIFY MARKING
- ⚠ REV.2 2022.04.01 | MODIFY P2 WORD MODEL & P1 VOLTAGE
- ⚠ REV.1.2021.12.13 | MODIFY CABLE LETTERING CONTENT

NOTE: Cable Length Unless Otherwise Spec. Tolerances: Under 6FT ±25mm; Another ±50mm